

AD FILE 1000

2

AD-A198 399

## REPORT DOCUMENTATION PAGE

2a. SECURITY CLASSIFICATION AUTHORITY		1b. RESTRICTIVE MARKINGS	
2b. DECLASSIFICATION/DOWNGRADING SCHEDULE		3. DISTRIBUTION/AVAILABILITY OF REPORT Approved for public release; distribution unlimited	
4. PERFORMING ORGANIZATION REPORT NUMBER(S)		5. MONITORING ORGANIZATION REPORT NUMBER(S) <b>AFOSR-TR- 88-0932</b>	
6a. NAME OF PERFORMING ORGANIZATION University of Florida	6b. OFFICE SYMBOL (If applicable)	7a. NAME OF MONITORING ORGANIZATION AFOSR/NP	
6c. ADDRESS (City, State and ZIP Code) Space Astronomy Laboratory 1810 N. W. 6th Street Gainesville, FL 32601		7b. ADDRESS (City, State and ZIP Code) Bldg 410 Bolling AFB DC 20332-6448	
8a. NAME OF FUNDING/SPONSORING ORGANIZATION AFOSR	8b. OFFICE SYMBOL (If applicable) NP	9. PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER F49620-83-C-0131	
8c. ADDRESS (City, State and ZIP Code) Bldg 410 Bolling AFB DC 20332-6448		10. SOURCE OF FUNDING NOS.	
11. TITLE (Include Security Classification) Shuttle Flight Test of an Advanced Gamma-Ray Detection System		PROGRAM ELEMENT NO 61102F	PROJECT NO 2309
12. PERSONAL AUTHOR(S) Alfred C. Rester, Jr.		TASK NO A1	WORK UNIT NO -
13a. TYPE OF REPORT Final	13b. TIME COVERED FROM 1 Jul 83 to 31 Jul 87	14. DATE OF REPORT (Yr., Mo., Day) 30 Jun 88	15. PAGE COUNT 16
16. SUPPLEMENTARY NOTATION			
17. COSATI CODES		18. SUBJECT TERMS (Continue on reverse if necessary and identify by block number)	
FIELD	GROUP	SUB. GR.	
		Gamma-Ray Detector, n-type Germanium Detector.	
19. ABSTRACT (Continue on reverse if necessary and identify by block number) The Gamma-Ray Advanced Detector (GRAD) is a gamma-ray detector systems consisting of a large-volume, n-type germanium detector with active shielding of bismuth germanate and plastic scintillators. It was diverted from the AFP-675 program to a balloon flight over Antarctica following the Challenger Disaster and the discovery the following year of the supernova 1987A. The present report outlines activities leading to and following the decision to go to Antarctica and summarizes the basic technological results from the project.			
20. DISTRIBUTION/AVAILABILITY OF ABSTRACT UNCLASSIFIED/UNLIMITED <input checked="" type="checkbox"/> SAME AS RPT. <input type="checkbox"/> DTIC USERS <input type="checkbox"/>		21. ABSTRACT SECURITY CLASSIFICATION <b>E</b> Unclassified	
22a. NAME OF RESPONSIBLE INDIVIDUAL Lt Col Bruce Smith		22b. TELEPHONE NUMBER (Include Area Code) 202-767-4908	22c. OFFICE SYMBOL NP

DTIC  
ELECTE

AUG 26 1988

**Final Report**

**Shuttle Flight Test of an Advanced Gamma-Ray  
Detection System**

**Dr. Alfred C. Rester, Jr.  
Principal Investigator  
University of Florida  
Laboratory for Astrophysics and Planetary Exploration  
One Progress Boulevard  
Box 33  
Alachua, FL 32615**

**Sponsored by**

**Advanced Research Projects Agency (DoD)  
ARPA Order No. 4565**

**Monitored by AFOSR under Contract No. F48620-83-C-0131**

**The views and conclusions contained in this document are those of the authors and should not be interpreted as necessarily representing the official policies, either expressed or implied, of the Defense Advanced Research Projects Agency or the U.S. Government.**

**June 30, 1988**

### Abstract

The Gamma-Ray Advanced Detector (GRAD) is a gamma-ray detector system consisting of a large-volume, n-type germanium detector with active shielding of bismuth germanate and plastic scintillators. It was diverted from the AFP-675 program to a balloon flight over Antarctica following the Challenger Disaster and the discovery the following year of the supernova 1987A. The present report outlines activities leading to and following the decision to go to Antarctica and summarizes the basic technological results from the project.

Accession For	
NTIS GRA&I	<input checked="" type="checkbox"/>
DTIC TAB	<input type="checkbox"/>
Unannounced	<input type="checkbox"/>
Justification	
By	
Distribution/	
Availability Codes	
Dist	
Special	
A-1	

## 1. Introduction

The Gamma Ray Advanced Detector (GRAD) (Refs 1,2,3) consists of an n-type germanium detector inside a closed-ended bismuth germanate annulus with additional plastic active shielding across the aperture. The detector was designed to be utilized as a gamma-ray telescope in the payload bay of the Space Shuttle. The technological goals of the GRAD included the evaluation of n-type germanium (nGe) and bismuth germanate (BGO) crystals as detectors in the environment of space and a study of the dynamic background in near-earth orbit. The major scientific objective was observation of the Galactic Center for evidence of the resurgence of a 511-keV gamma-ray source (4) which was last seen earlier in this decade.

Originally scheduled for launch in 1986 as a part of the AFP-675 Program on the first Space Shuttle flight out of the new Vandenberg Launch Facility, flight of GRAD and its sister experiments on AFP-675 were postponed for an indeterminate time on account of the Challenger Disaster. In the aftermath of the tragedy we investigated several options for flight other than AFP-675, should that program be unacceptably delayed by the disruption.

In the meantime the arrival of emissions from the supernova 1987A (5), the first of such magnitude to occur in 400 years, presented us with a target of opportunity having ideal technological characteristics and of

monumental scientific importance. Visible from the Southern Hemisphere, this object promised to provide us with the opportunity of not only testing the sensitivity of our detector system but verifying the hypothesized sites of nucleosynthesis of the heavy elements as well. In order to take advantage of this rare opportunity we began preparations for what would be a successful flight of GRAD from Antarctica on a high-altitude balloon launched by the Air Force Geophysics Laboratory. Early feasibility studies for the Antarctic mission were performed under the present contract; major modifications to GRAD, testing and mission operations were carried out under a later grant through the Office of Naval Research, which is a participant in the Florida Demonstration Project.

## 2. The GRAD Spectrometer

A complete description of the GRAD is provided in Refs. 1-3. In passing we note that its central detector is a 5.5 cm x 5.7 cm nGe crystal with an energy resolution of 2 keV at 1332 keV. This cylindrical detector is cooled with a space qualified liquid nitrogen dewar with a holding time of 21 days. As can be seen in Fig. 1, it is enclosed in active shielding of bismuth germanate on all sides but the top, where the 60-degree (full angle) aperture is covered with a thin plastic scintillator to veto charged particle induced events without appreciably attenuating the incoming gamma-ray. The shield also has excellent Compton suppression characteristics, as can be seen from the laboratory measurements shown in Figure 2. Because the purpose of the AFOSR contract was the testing of new detector technology in the environment of Space we include here in Fig. 3 an actual measurement of the total (particle plus gamma-ray) background rejection as

a function of energy, taken at 118,000 feet over Williams Field, Antarctica on January 8, 1988. Background suppression factors of about 20 are clearly evident.

Prior to the mission we estimated the sensitivity curve shown in Figure 4, assuming a background continuum intermediate to that of the HEAO-C and Apollo 15 gamma-ray detectors. It is interesting in retrospect to compare the predicted sensitivity with the gamma-ray fluxes from the supernova 1987A measured with GRAD on the Antarctic balloon flight. We note that the spectrometer was not only sensitive enough to detect these weak signals in the high radiation background over Antarctica, but provided the first detection of the weak 2598-keV gamma ray from the beta decay of Co-56 as well as the first measurement ever reported of Doppler line broadening and splitting in supernova gamma rays.

### 3. Modifications required for balloon flight

During the early spring of 1987 we began to assess the modifications required to redirect the GRAD experiment from the Space Shuttle to Antarctic balloon flight. In the main the changes required included the development of interface and communications boards, a mechanical support structure, a pressurized housing for the top of the detector, and new software to support an experiment controlled from the ground rather than from the aft flight deck of the Orbiter. In addition we had to install new timing circuitry to improve the background suppression of the detector.

3.1 Thermal Design. The GRAD thermal subsystem includes its own heaters and thermostats, as there were none on the EES mounting surface for AFP-675. NASA/GFSC performed thermal modelling studies to ascertain what changes would be required for the balloon-borne system.

3.2 Mechanical Design. Although GRAD was designed to operate in the hard vacuum of space, some modifications were necessary for operation at 120,000 feet. These entailed encapsulation of the high voltage power supplies to prevent coronal discharge. This was accomplished by a combination of potting and enclosure with an airtight housing over the detector elements. Gaseous nitrogen vented from the liquid nitrogen dewar was circulated through the enclosure at one atmosphere of pressure to keep the ambient pressure in the neighborhood of the high voltage supplies above the coronal discharge point. Pointing was accomplished by fixed declination and an existing azimuthal pointing system available through AFGL.

A consideration peculiar to the search for evidence of the  $^{56}\text{Ni}$  decay chain in the supernova spectrum was the necessity of reducing possible man-made sources of these lines in the vicinity of the gamma-ray detector. Structural materials containing Fe, Co, Ni, or possibly Cu which could yield significant quantities of these isotopes in compound nuclear reactions with protons were therefore undesirable. Except for some steel bolts on the exterior of the shield, the structural materials holding the detector elements together were almost entirely of Al; we replaced these bolts with titanium fasteners.

### 3.3 Electrical Design.

3.3.1 Electrical accommodations. Approximately 11 kWh of electrical power at a nominal 28 VDC was required for 72 hours of operation. This was supplied by batteries.

### 3.3.2 Modifications to GRAD Avionics and GSE.

#### A. Software modifications

1. Serial command interface
2. Data storage during loss of communications
3. Packaging and synchronization of data in telemetry stream.
4. Interrupt handling

#### B. Hardware modifications

1. Redesigned telemetry board for standard balloon telemetry interface.
2. Adapted existing ground test serial interface
3. Expanded system memory for data buffering
4. Installed improved timing circuitry.

#### C. Ground Support Equipment (GSE) modifications

##### 1. Software

- a. command formatter
- b. ancillary data message handler
- c. real time data reception and storage



## 2. Hardware

- a. redesigned spacecraft simulator board to convert ground support equipment to ground control system
- b. installed second CPU for data reception and storage.

3.4 Testing and Checkout. GRAD had to undergo complete mechanical and electrical testing prior to shipping to Antarctica. The requirements for balloon flight were less stringent than those met for spaceflight; however the unique conditions prevailing at the South Pole posed additional requirements.

The majority, if all, of the testing was accomplished at Holloman AFB.

3.5 Safety. GRAD was already safety certified for flight on AFP-675; safety requirements for balloon flight were less stringent. An onboard radioactive calibration source of about 2 microcuries strength was to be removed from the payload in order to reduce the background level and eliminate the possibility of loss in the Antarctic environment, should the payload not have been recovered. The space in the memory devoted to storage of calibration spectra was used instead to log the occurrence of single-event upsets and their subsequent correction, a valuable record for the assessment of the performance of the radiation hardened software.

#### 4 Results.

Although the eventual flight of the GRAD turned out to be under radically different circumstances than originally scoped before the Challenger disaster, quick response to an unusual opportunity allowed us to make a timely flight with the instrument and accomplish its objectives several years earlier than would have been possible had we waited for the resumption of Space Shuttle flights. Some of the early performance data have been presented above. A more complete analysis is underway, but the basic conclusions can already be stated.

1. Bismuth germanate has fewer activation lines in its background than sodium iodide or cesium iodide. It suppresses unwanted background efficiently.
2. The weight and volume savings of BGO over the conventional active shielding materials is real. Early comparison of results with those of workers using a sodium iodide appears to indicate that the 80-lb BGO shield performed as well as an 800-lb shield of sodium iodide.
3. The n-type germanium detector performed well. However it was not in the space environment long enough for us to assess the rate of accumulated radiation damage, as it was negligible.
4. The hybrid design of the spectrometer functioned according to design expectations.

5. Neutron interactions in the germanium detector proved to be an important limiting factor in signal-to-noise ratio. That this is so is due at least to the very good background noise suppression of the system.

6. The computer code RCOLD and its advanced form ROBFIT functioned very well in the extraction of signals so weak that they are nearly buried in the noise. This pattern recognition approach to spectral analysis may have important practical applications.

### References

1. A. C. Rester, R. B. Piercey, G. Eichhorn, R. L. Coldwell, J. McKisson, D. W. Ely, H. M. Mann and D. A. Jenkins, IEEE Trans Nucl. Sci. 33, 732 (1986)
2. R. B. Piercey, J. McKisson, G. Eichhorn, A. C. Rester and H. M. Mann, IEEE Trans. Nucl Sci 33, 866 (1986)
3. G. Eichhorn and R. B. Piercey, IEEE Trans. Nucl. Sci. 33, 1100 (1986)
4. M. Leventhal and C. J. McCallum, AIP Conf. Proc. 101, Ch. IV, pp 211-229
5. I. Shelton, reported by W. Kunkel and B. Madore, IAUC 4316, 1987 February 24..

### List of Figures

1. The GRAD Gamma-Ray Spectrometer.
2. Laboratory measurement of rejection of Compton-scattered gamma rays.
3. Comparison of GRAD background spectrum with BGO shield enabled (lower background spectrum) and disabled (higher background) taken over Antarctica on a balloon flight of 8 January 1988.
4. Estimated sensitivity of GRAD spectrometer for the detection of weak lines. The points represent actual supernova lines detected with the instrument.

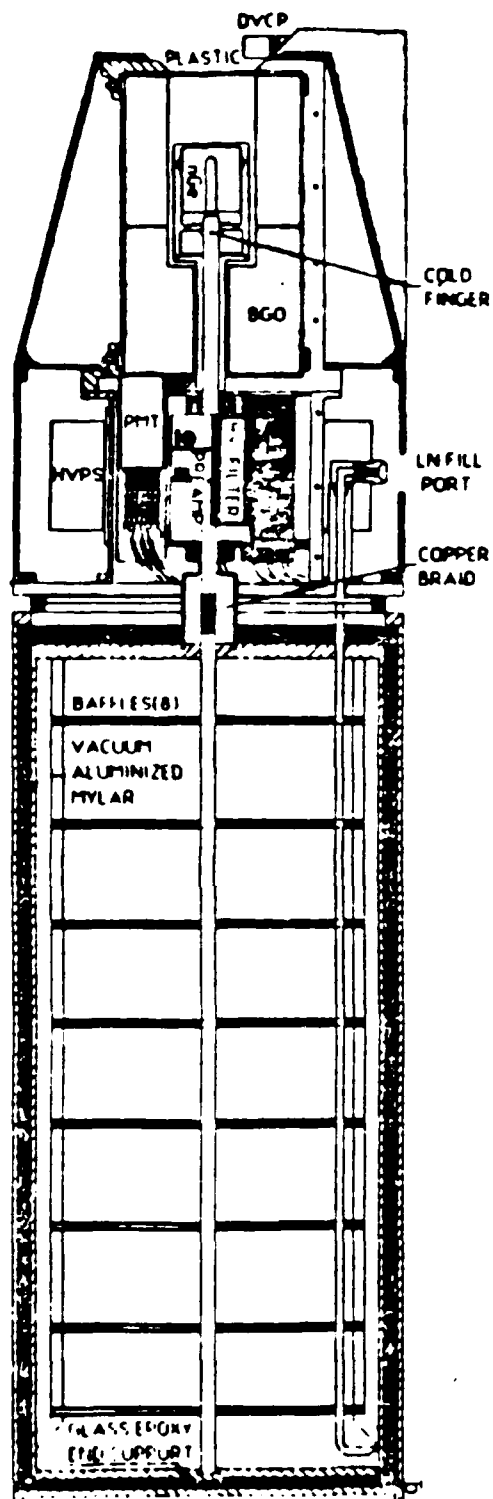


Figure 1. The Gamma Ray Advanced Detector (GRAD)

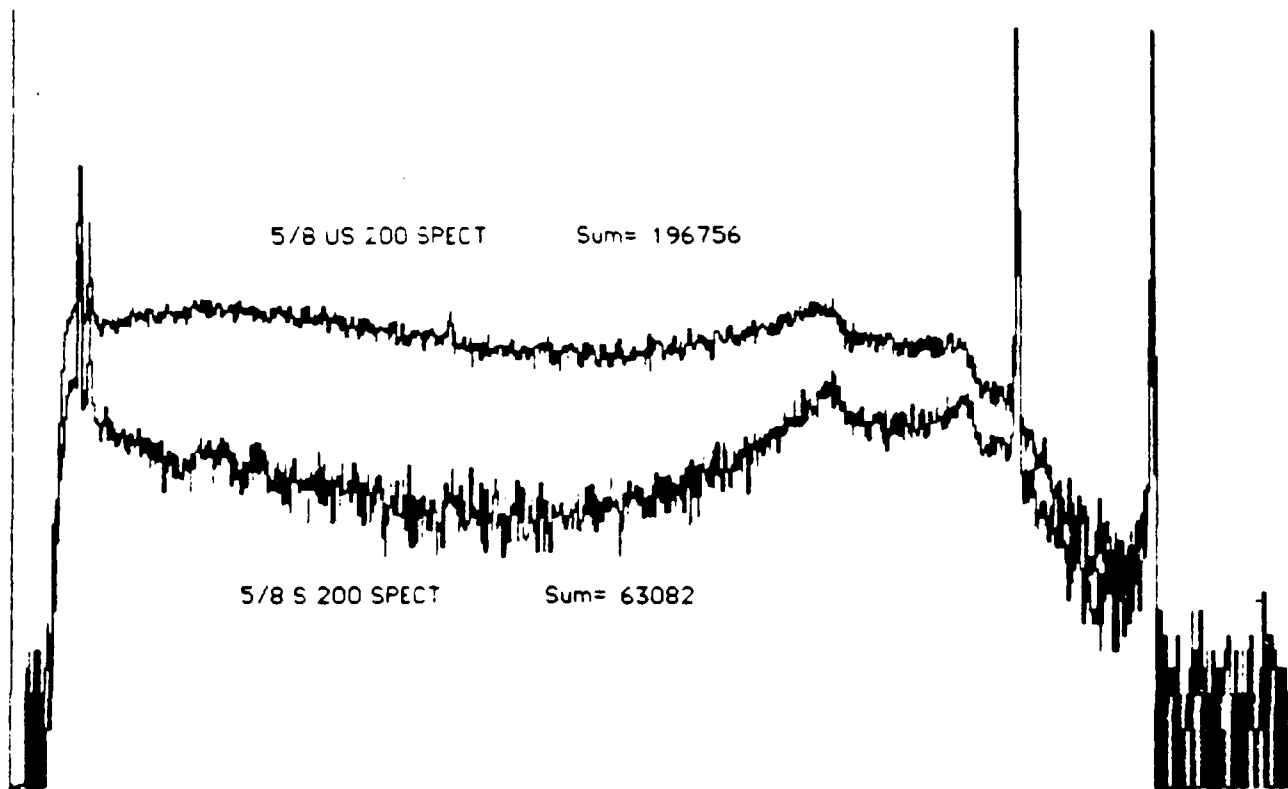


Figure 2. Compton Suppression of BGO shield.  
Upper spectrum: shield off.  
Lower spectrum: shield on.

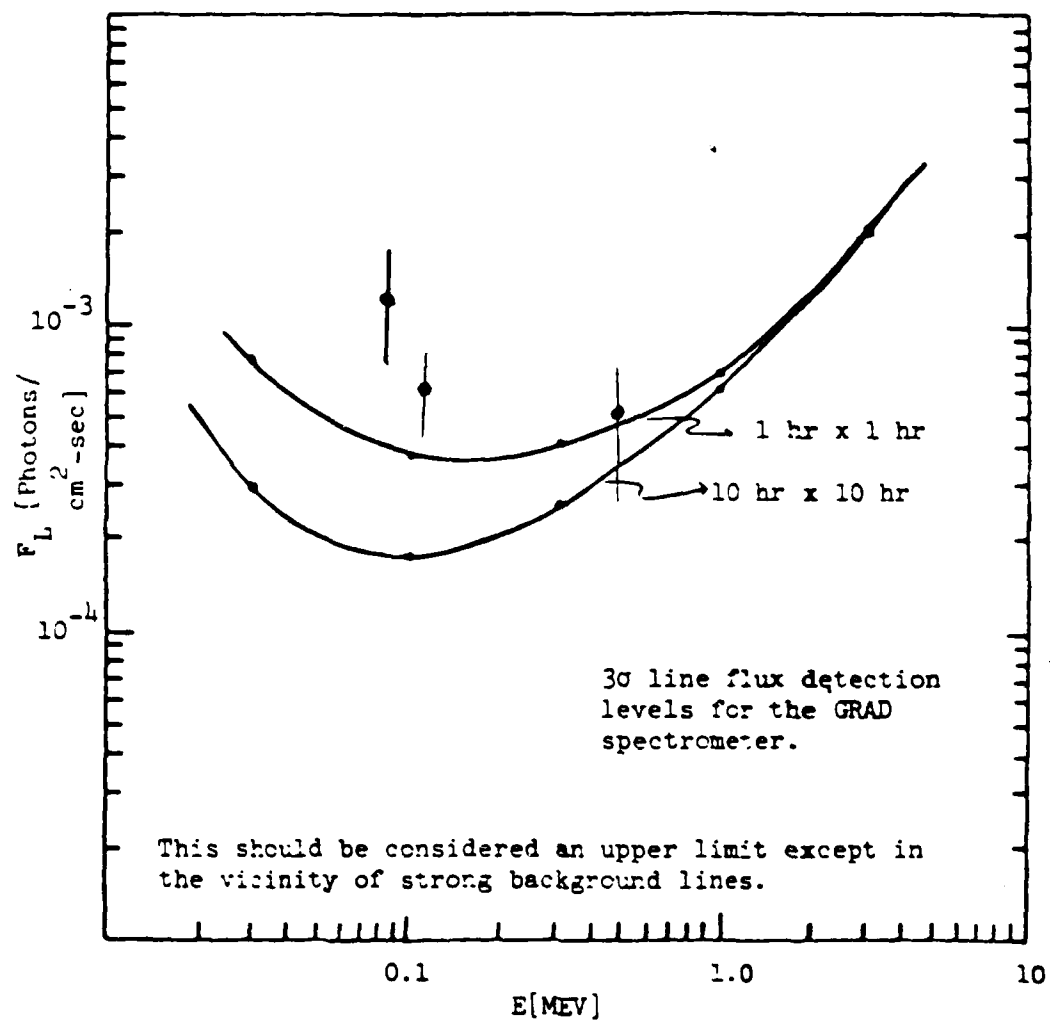


Figure 4. Estimated sensitivity of GRAD spectrometer for the detection of weak lines. The points represent actual supernova lines detected with the instrument.



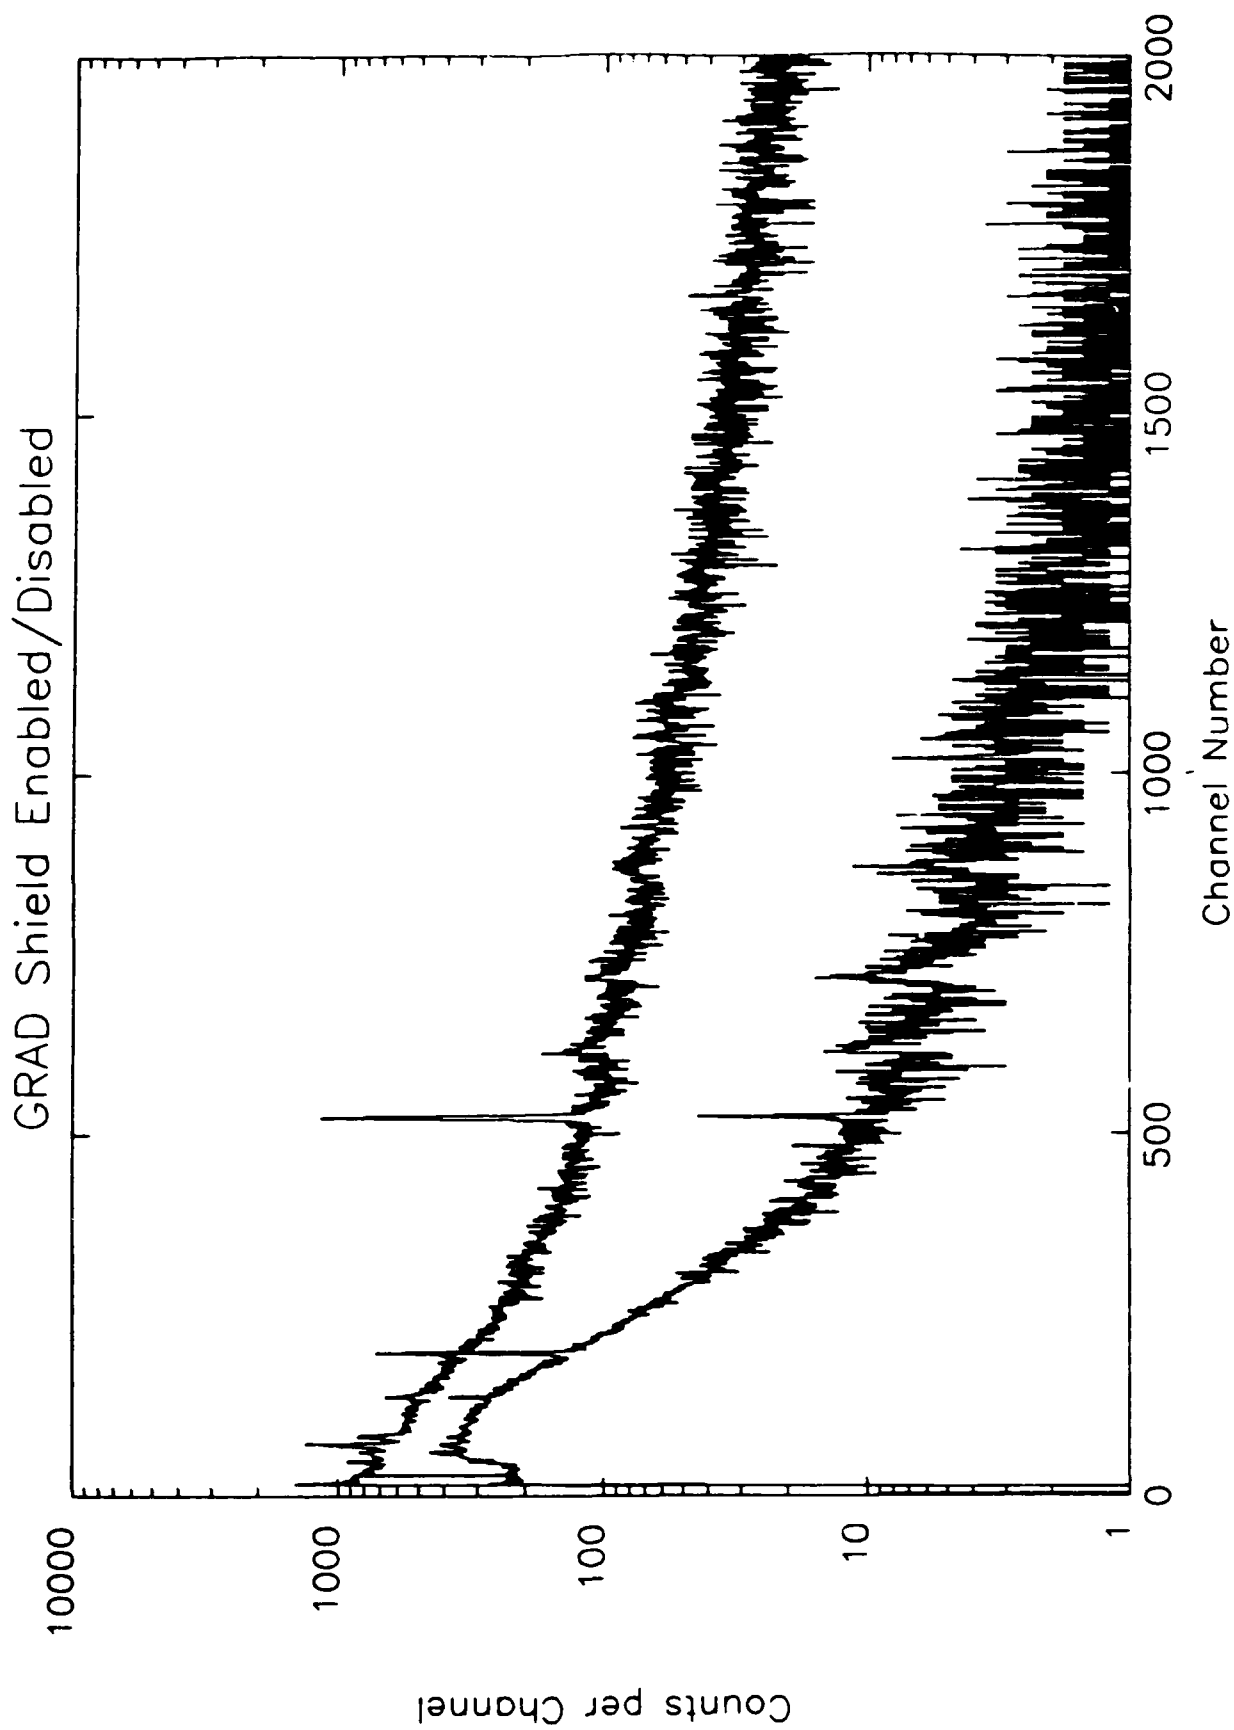


Figure 3. GRAD background spectrum taken over Antarctica on 8 Jan 1988